

Centrifuge 5417 C / R



eppendorf



Fig. 1



Fig. 2

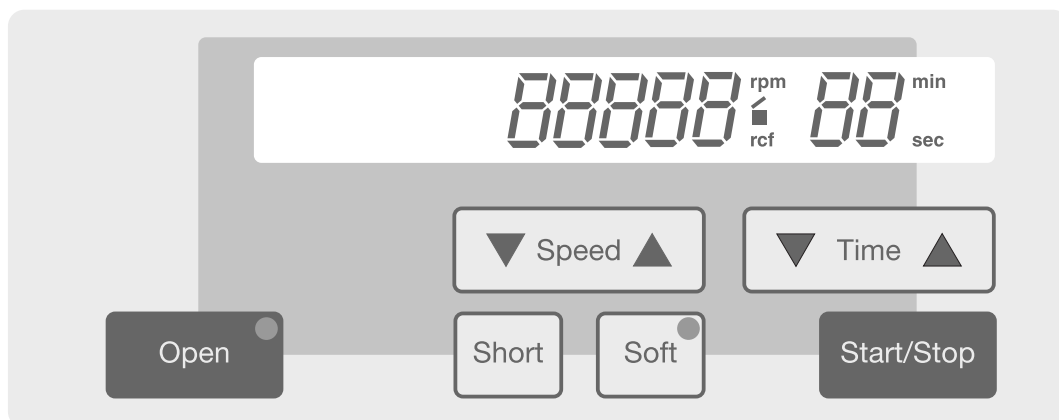


Fig. 3

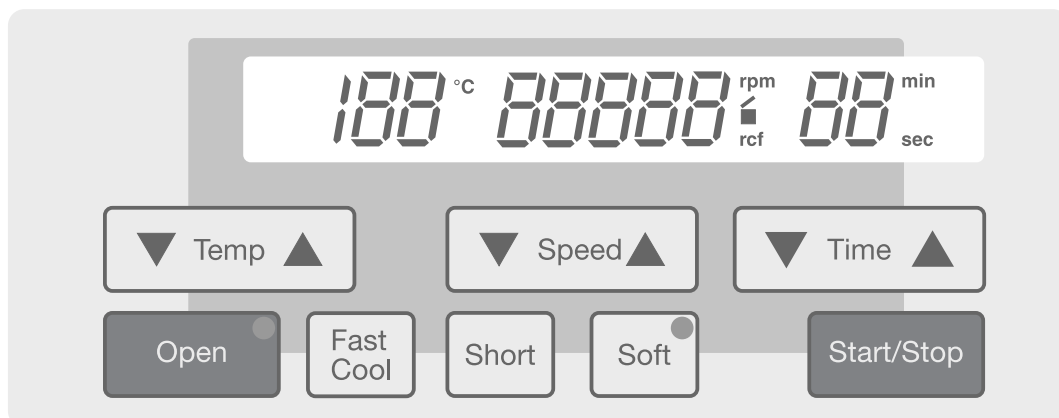


Fig. 4

Contents

1	Introduction	18
1.1	Delivery package	18
1.2	Unpacking	18
1.3	Installing the device	18
2	Safety	19
2.1	Intended use	19
2.2	Safety precautions and applicational limitations	19
3	Operation	21
3.1	Operating controls	21
3.2	Rotor description	21
3.3	Mounting / dismounting the rotors	22
3.4	Loading the rotors	22
3.5	Routine centrifugation with preset time / rcf display	22
3.6	Continuous operation	23
3.7	Short spin centrifugation	23
3.8	Centrifugation with Soft start / stop	24
3.9	Refrigeration (for 5417 R only)	24
3.10	Automatic rotor recognition	24
3.11	Display of nominal value during the run	24
3.12	Display of elapsed spin time	25
3.13	Control via serial interface (optional)	25
3.14	Opening the centrifuge in the case of a power failure	25
3.15	Fuses	25
4	Maintenance and cleaning	26
4.1	Device	26
4.2	The rotors	26
4.3	Aerosol-tight rotors	26
4.4	Rotor sterilization	26
4.5	Refrigerated centrifuges	26
4.6	Glass breakage	27
4.7	Return the device	27
5	Troubleshooting	28
6	Technical data	29
7	Ordering information	30
8	Appendix	32

1 Introduction

Centrifuge 5417 C is a non-refrigerated bench-top centrifuge and Centrifuge 5417 R is a refrigerated bench-top centrifuge. In both devices, Eppendorf Micro Test Tubes can be centrifuged at 20,800 rcf (14,000 rpm). It is possible to attain an rcf of up to 25,000 using a special 24-position rotor. For special applications, a swing-bucket rotor is available with 8 positions for centrifuging Eppendorf Micro Test Tubes at a maximum rotational speed of 10,500 rpm (11,700 rcf). PCR tubes can be centrifuged in a rotor which can accommodate six 8-tube strips.

Before starting up Centrifuges 5417 C / R for the first time, please read the operating manual and observe the safety regulations.

1.1 Delivery package

- 1 Centrifuge 5417 C with fan cooling or 1 Refrigerated Centrifuge 5417 R (rotor not included with centrifuges)
- 1 Mains cable
- 1 Operating manual
- 1 Hexagonal key
- 2 Spare fuses

1.2 Unpacking

When removing the centrifuge from the packaging, take hold of it at the sides, support it from underneath and lift it onto the lab bench.

1.3 Installing the device

Remove the transport safety devices according to the instructions on the pack insert and save these for possible future transport of the centrifuge. Only tilt the device slightly; do not place it on its side!

 **For 5417 R only: To avoid damage to the compressor caused by incorrect transportation, wait four hours after installation before switching on the device.**

To disconnect the mains supply from the centrifuge in the event of errors occurring, an emergency switch which is separate from the centrifuge must be available. This switch should be outside the room in which the centrifuge is operated or next to the exit of the room.

Before plugging in the centrifuge, check that the mains voltage and frequency corresponds to the specifications on the identification plate of your centrifuge. The mains connection of the centrifuge may only be connected to a socket with a protective conductor.

Place the centrifuge onto a stable, vibration-free, horizontal surface. Make sure that the centrifuge is not exposed to direct sunlight. To ensure sufficient ventilation, there should be clearance of 15 cm on both sides of the centrifuge to the wall or other devices. This is particularly important for the refrigeration function of Centrifuge 5417 R. According to recommendations of the EN 61010-2-020 standard, a safety distance of 30 cm should be observed around the centrifuge during operation. No objects whose destruction may cause damage should be positioned in this space.

Connect the centrifuge to the mains supply and press the mains switch. The switch is located on the rear of the device (5417 C) or on the right-hand side of the device, directly next to the mains connection. The centrifuge lid can now be opened by pressing **Open**. Insert the rotor before starting **and tighten**.

Please remove the protective strip from the display.

Do not move or knock against with the centrifuge during operation.

2 Safety

2.1 Intended use

Eppendorf centrifuges serve to separate components of mixtures of different densities, especially for the preparation and processing of samples from the human body within the scope of in-vitro diagnostic applications, in order to allow the in-vitro diagnostic medical device to be used as intended. Therefore centrifuges, being in-vitro diagnostic accessories, are in themselves in-vitro diagnostic medical devices within the meaning of Directive 98/79/EC of the European Parliament and of the Council of 27 October 1998 on in-vitro diagnostic medical devices.

Eppendorf centrifuges are intended for indoor use only.

This device may only be operated by trained specialist staff.

2.2 Safety precautions and applicational limitations

In the interest of your own personal safety, always observe the following regulations:



The rotor and the rotor lid must always be securely fastened.

Do not begin centrifugation before the rotor has been securely fastened.

Do not use buckets and rotors which show clear signs of corrosion or mechanical defects. Please check the accessories at regular intervals.

The rotor must be loaded symmetrically. Opposing tubes should be of the same type and should be filled equally.

Please use only the original accessories recommended.

Do not move or knock against the centrifuge during operation.

Repairs must only be performed by an Eppendorf authorized service technician. Only use original rotors and spare parts recommended by Eppendorf.

Do not operate centrifuges which have not been correctly installed or repaired.

Centrifuges 5417 C and 5417 R may only be used for specified applications. They must not be operated in a hazardous or potentially flammable environment and must not be used to centrifuge explosive or highly reactive substances.

When handling toxic, aggressive or radioactive liquids or pathogenic bacteria out of Risk Group II (see World Health Organization: "Laboratory Biosafety Manual"), observe national regulations.

Fluids or materials used for cleaning and disinfecting should be disposed of in accordance with approved laboratory regulations.

If aggressive liquids are spilled in the rotor or rotor chamber, the centrifuge must be cleaned ***immediately*** with a moist cloth and a mild soap solution. This is particularly important for the bores of the fixed-angle rotors.

A liquid density of 1.2 g/ml must not be exceeded at the maximum rotational speed.

During longer spin times in the non-refrigerated Centrifuge 5417 C, the sample tubes may heat up. Observe the limiting data specified by the tube manufacturer.

The use of organic solvents and reagents (e.g. chloroform, phenol) may have an adverse effect on the stability of plastic test tubes and may attack the plastic rotor boiler.

Following operation in a cool room, run the centrifuge for 30 minutes in the cool room until it is warm. Alternatively, allow it to warm up in a lab for at least three hours, but ***do not plug in the centrifuge during this period*** in order to prevent damage caused by condensation.

Rotors are high-grade components which are subject to extreme mechanical strain. Aluminium rotors are protected against corrosion caused by commonly-used laboratory chemicals by means of an electrolytic coating, although this protection cannot be fully guaranteed.

Please ensure that the rotor is protected from mechanical damage. Even slight scratches and cracks can cause severe inner damage to the rotor materials.

Prior to centrifugation, the tubes should in any case be visually inspected for material damage. Damaged tubes may not be centrifuged. This is because broken tubes can, in addition to sample loss, result in further damage to the centrifuge and accessories.

Please avoid using aggressive chemicals with the rotors. Such chemicals include concentrated and mild alkalis, concentrated acids, solutions containing mercury ions, copper ions and other heavy-metal ions, chlorinated hydrocarbons and concentrated saline solutions. If such chemicals come into contact with the rotor, clean the rotor and the rotor bores ***immediately!***

Please clean your rotor regularly using a ***neutral*** cleaning liquid (e.g. Extran® neutral or RBS neutral). This will protect the rotor and maintain its service life.



Do not use rotors, lids and buckets which have been damaged by chemicals or as a result of mechanical faults!

Transfer

If the device is passed on to someone else, please include the instruction manual.

Disposal

In case the product is to be disposed of, the relevant legal regulations are to be observed.

Information on the disposal of electrical and electronic devices in the European Community

The disposal of electrical devices is regulated within the European Community by national regulations based on EU Directive 2002/96/EC on waste electrical and electronic equipment (WEEE).

According to these regulations, any devices supplied after 13.08.05 in the business-to-business sphere, to which this product is assigned, may no longer be disposed of in municipal or domestic waste. They are marked with the following symbol to indicate this.



As disposal regulations within the EU may vary from country to country, please contact your supplier if necessary.

3 Operation

3.1 Operating controls

Please open up the fold-back cover at the front and back of this manual.

- Fig. 1: Front of 5417 R with emergency lid release E (see 3.14)
- Fig. 2: Rear of 5417 C with switch and fuse insert
- Fig. 3: Display and control panel of 5417 C
- Fig. 4: Display and control panel of 5417 R
- Fig. 5: Fixed-angle rotor for 30 / 24 positions
- Fig. 6: Swing-bucket rotor
- Fig. 7: Rotor for 8-tube strips for PCR test tubes

3.2 Rotor description

Standard rotor F-45-30-11

The standard rotor **F-45-30-11** is a **fixed-angle, 45 degree** rotor with **30** positions of **11 mm** diameter each. 1.5 ml and 2.0 ml tubes can be inserted directly. With adapters, 0.5 ml and 0.4 ml centrifuge tubes as well as 0.2 ml PCR tubes can be used.

The standard rotor can be operated up to a maximum of 14,000 rpm, with an rcf of 20,800.

The O-ring inserted into the rotor reduces the noise made by the centrifuge; it is not a sealing ring.

A replacement O-ring is included in the delivery package.

The rotor lid, which should always be attached during centrifugation, is fastened by pressing down the button and rotating to the right.

Aerosol-tight rotor FA-45-30-11

The aerosol-tight rotor **FA-45-30-11** has the same technical data as the standard rotor. The rotor lid is made of aluminium and is tightened with a threaded knob.

The rotor lid and the lid screw are provided with a silicone seal which prevents the escape of aerosols from the rotor chamber. The sealing ring must be kept clean and the lid must be properly fastened.

Aerosol-tight rotor F-45-24-11

This rotor can accommodate 24 tubes for 1.5 ml or 2.0 ml and can produce an rcf of 25,000 (16,400 rpm). The aerosol-tightness of the a lid can be guaranteed by tightening the threaded knob.

Rotor lid and seals are subject to natural wear and tear and should be replaced when worn.

Aerosol-tightness has been tested and approved in accordance with the procedure of Bennett *et al.* from the Centre for Applied Microbiology & Research, CAMR, Porton Down, Great Britain, and according to Annex AA of the IEC 1010-2-020 safety standard. (Certificate <http://www.eppendorf.com>).

The lid of aerosol-tight rotors must not be fastened tightly during storage!

Swing-bucket rotor A-8-11

Swing-bucket rotor A-8-11 contains eight swing buckets for 1.5 or 2.0 ml tubes. Adapters allow 0.5 ml, 0.4 ml or 0.2 ml tubes to be used.

The maximum permitted speed is 10,500 rpm (5417 R), effecting a relative centrifugal force of 11,700 x g.

Maximum speed on the 5417 C: 10,000 rpm, corresponding to a relative centrifugal force of 10,600 x g.

Speed is limited automatically on Centrifuge 5417 C / R (see Item 3.10).

Please check that all swing buckets are properly suspended and can swing freely with the tubes.

PCR-tube strip rotor F-45-48-PCR

This rotor can accommodate six 8-tube strips or six 5-tube strips for 0.2 ml PCR test tubes or 48 individual PCR test tubes.

The maximum permitted speed is 10,500 rpm (5417 R), effecting a relative centrifugal force of 11,700 x g.

Maximum speed on the 5417 C: 10,000 rpm, corresponding to a relative centrifugal force of 10,600 x g.

3.3 Mounting / dismantling the rotors

Clean the motor axle and the rotor bores with a cloth before attaching the rotor.

- Mount the rotor onto the motor axle and tighten the rotor nut by turning it clockwise using the hexagonal key supplied.
- To dismount the rotor, turn the rotor nut counterclockwise using the hexagonal key.
- The aerosol-tight rotor can also be removed from the centrifuge when the lid is closed; this is done by inserting the hexagonal key into the opening in the lid screw. This can be useful when the tubes are removed on a clean-room bench.
- Do not centrifuge using rotors and buckets with visible corrosion or mechanical defects.

3.4 Loading the rotors

The rotors and buckets must always be loaded symmetrically. The adapters may only be loaded with the test tubes recommended.

Differences in the weight of the filled sample tubes should be kept as low as possible in order to prolong the lifetime of the drive and to minimize running noise.

The maximum permitted weight of a filled bucket is stated on each rotor. This weight must not be exceeded when the buckets are filled completely (see Section 2, "Safety regulations and applicational limitations").

Swing-bucket rotor:

For reasons of mechanical stabilization, **all** positions must be loaded with buckets of the same type.

Ensure that the grooves are clean before inserting the buckets.

Unclean grooves and pivots prevent the buckets from swinging freely. The plastic buckets should not be lubricated.


3.5 Routine centrifugation with preset time / rcf display

Switch on the mains supply. The nominal values of the last run appear in the display.

Load the rotor **symmetrically** and close the centrifuge lid. The green lamp in the **Open** key lights up. If "LID" lights up in the display field, close the lid again.




To modify the values for the rotational speed / rcf (relative centrifugal force), time and temperature: The new nominal value appears in the display.



When both arrow keys are pressed simultaneously, the centrifuge switches from "rpm" (rotational speed) to "rcf". The rcf symbol appears in the display.



To set the run time (minutes / seconds). The remaining centrifugation time is displayed in minutes, with the last minute being counted down in seconds. When the time is changed during the run, the time which has elapsed is included in the calculation of the new actual value.




To set the temperature preselection.



To start or end the run. ■ flashes for as long as the rotor is spinning.



To open the lid when the control lamp in the key is lit up. The  symbol shows that the rotor is not moving.

During the run, the rotational speed of the rotor or the appropriate rcf value, the sample temperature and the remaining spin time in minutes are displayed. During the run, all parameters can be modified.

After the end of a run, or after a run has been interrupted by pressing the **Stop** key, the rotor is braked and brought to a standstill. During the braking process, the time display flashes and the elapsed spin time is displayed.

3.6 Continuous operation



The continuous operation function is set above 99 min or below 10 sec using the **arrow keys**. In the time display, "oo" indicates continuous operation.

During the run, the actual values for temperature, rpm/rcf and the elapsed time (in minutes) are displayed. If the centrifuge runs for longer than 99 minutes, "99" flashes.



To start / end the run.

3.7 Short spin centrifugation



This key should be held down for the intended duration of the run. The time which has elapsed is displayed in seconds. A run which has already been interrupted can be restarted by pressing the key again, provided that the centrifuge has not come to a standstill.

Runs with a duration of 10, 20 or 30 seconds may be set using the time selection.

If the **Short** key is pressed when the lid is open, one of the following six status displays appears:

"10 t" or "1-10 t" / "14 t" or "1-14 t"/"16 t" or "1-16 t".

If the key is held down for longer than three seconds, the device switches to the other status and displays this for two seconds. The way which was last set is retained and appears in the display.

The meaning of the status displays is as follows:

"10 t": The swing-bucket rotor runs to its maximum speed of 10,000 rpm (5417 R)

"14 t": The 30-position fixed-angle rotor runs to its maximum speed of 14,000 rpm

"16 t": The 24-position fixed-angle rotor runs to its maximum speed of 16,400 rpm

"1-10 t": The speed can be selected with the cursor keys (swing-bucket rotor)

"1-14 t": The speed can be selected with the cursor keys (30-position fixed-angle rotor)

"1-16 t": The speed can be selected with the cursor keys (24-position fixed-angle rotor)


3.8 Centrifugation with Soft start / stop



When this key is pressed before or during acceleration, the acceleration and braking phase is extended to approximately 60 sec. This is indicated by the control lamp in the key.

The Soft mode cannot be switched off after acceleration has finished.

3.9 Refrigeration (for 5417 R only)



The nominal temperature can be set from $-9\text{ }^{\circ}\text{C}$ to $+40\text{ }^{\circ}\text{C}$. It can also be modified during the run.

Once the nominal temperature set has been reached, a deviation greater than $\pm 3\text{ }^{\circ}\text{C}$ is indicated by a flashing temperature display.

If the temperature deviates by more than $5\text{ }^{\circ}\text{C}$, the centrifuge switches off with a periodic warning signal.



To start a temperature-control run at a rotor-specific speed.

Refrigeration enables the new, preset temperature *in the rotor* to be reached rapidly. The run ends automatically or by pressing the **Stop** key. A periodic warning signal is emitted. Cooling from RT to $4\text{ }^{\circ}\text{C}$ lasts approximately 20 minutes.

Standby-refrigeration

When the lid is closed, the rotor chamber is refrigerated to the preselected nominal temperature before or after a run as long as this value is below ambient temperature. The rotor does not spin during this procedure and the temperature is adjusted more slowly. The nominal temperature appears in the display.

To protect the device, refrigeration switches off automatically if the centrifuge is not used for longer than six hours or if the lid is not opened. **Standby off** and the actual temperature in the chamber appears in the display. The desired temperature can be reached again quickly via **Fast Cool**.

Please empty and clean the tray for condensation water (located below the device) at regular intervals. This tray can be removed by pulling it out towards the front.



Please remove condensation water or ice (by thawing) from the rotor chamber at regular intervals. This should be carried out using a soft, absorbent cloth.

Note: If room temperature is lower than $18\text{ }^{\circ}\text{C}$, a warm-up time of approximately one hour is necessary to guarantee problem-free operation.

3.10 Automatic rotor recognition

Rotor recognition occurs at the beginning of every run. If the maximum rotational speed of the rotor is lower than the nominal rotational speed after a rotor has been exchanged, the run is interrupted. **SPEED** appears in the display.

The new maximum rotational speed appears in the display. New nominal values up to this rotational speed may be set.

3.11 Display of nominal value during the run

If an arrow key is pressed when the centrifuge is running, all nominal values are displayed for three seconds. The nominal value changes each time the key is pressed within this period.

3.12 Display of elapsed spin time

If both **Time** arrow keys are pressed simultaneously, the total run time of the centrifuge (in hours) appears in the display. This function can only be called up when the lid is open.


3.13 Control via serial interface (optional)

With special centrifuge models (ordered in advance), all centrifuge functions can be operated via the serial interface (RS 232 C).

Only devices which have been tested in accordance with IEC 950 may be connected via the serial interface.

3.14 Opening the centrifuge in the case of a power failure

If the magnetic lid latch cannot be activated because of a power failure, the emergency lid release can be activated manually:

 Turn off the mains switch. Wait until the rotor has come to a standstill. Open the lid carefully, as the rotor may continue spinning for some time. Disengage the lid latch by pressing the lid down slightly.

A plastic knob is situated at the left front edge of the base plate (see Fig. 1, E). After this knob has been pulled out and then downwards, the emergency lid release can be activated. The lid latch is disengaged by pressing down the lid lightly. The knob must be then reinserted.

3.15 Fuses

The red fuse holder is located next to the mains cable port in the connection unit. If necessary, the fuse holder can be removed and the two fuses can be replaced (see "Ordering information").

Only use fuses which have the nominal values printed on the identification plate of the device (current intensity, slow).

					Order no.
For 5417 R	230 V:	2 x 6.3 A	T	5 x 20	5417 341.007
	120 V:	1 x 10.0 A	T UL	6.3 x 32	5417 357.000
	100 V:	1 x 12.0 A	mTUL	6.3 x 32	5407 356.006
For 5417 C	230 V:	2 x 6.3 A	T	5 x 20	5417 341.007
	120 V:	1 x 8.0 A	T UL	6.3 x 32	5417 356.004
	100 V:	1 x 10.0 A	T UL	6.3 x 32	5417 357.000

4 Maintenance and cleaning

4.1 Device



The outside of the centrifuge and the rotor chamber should be cleaned regularly with neutral detergent. This is for hygiene purposes as well as to prevent contamination caused by residual contamination.

The user is responsible for cleaning or decontaminating the centrifuge in the event of decontamination caused by high-risk substances.

Open the lid of the centrifuge and disconnect the mains plug. Unscrew the rotor with the hexagonal key provided and clean separately. Only **neutral** agents may be used for cleaning and disinfection (e.g. diluted Extran® **neutral**, RBS **neutral** or 70 % isopropanol/water mixture or an alcohol-based disinfectant). The rotor chamber should only be cleaned with a moist cloth.

After cleaning with detergent, the rubber seals in the rotor chamber should be rinsed **well with water** and lubricated with glycerine.

The user must consult the manufacturer before cleaning or decontaminating the centrifuge using methods not recommended by the manufacturer in order to ensure that the centrifuge is not damaged.

To ensure that the centrifuge functions correctly and safely in the long-term, please note that aggressive chemicals can damage the rotor, buckets and boiler. Please check the centrifuge regularly for damage caused by corrosion.

4.2 The rotors

The rotor and buckets must be cleaned regularly to prevent contamination caused by residue. Check the rotor and housing **monthly** for residue and corrosion. This applies in particular to the rotor bores. Please clean your rotor using a neutral cleaning liquid. This will protect the rotor and maintain its service life. As a reminder, the message "CLEAn ro" appears in the display of the centrifuge three times after every 200 runs.

The magnetic ring on the base of the rotor is for rotor recognition and rotational speed monitoring. If damaged, it must be replaced by a service technician.



Do not carry out centrifugation using damaged rotors.



4.3 Aerosol-tight rotors

The lid of the aerosol-tight rotors FA-45-30-11 and F-45-24-11 should be replaced in the event of excessive wear and tear. To protect the rotor, please ensure that the sealing rings are maintained regularly.

The lid of the aerosol-tight rotor must not be fastened tightly during storage!

4.4 Rotor sterilization

All rotors are autoclavable (121 °C, 20 min).

After the rotor has been autoclaved a maximum of ten times, the lids of the aerosol-tight rotors must be replaced.

4.5 Refrigerated centrifuges

Please remove any condensation water in the rotor chamber using a soft, absorbent cloth.

Switch off the centrifuge after use, leave the lid open and empty the tray for condensation water, located below the device. The tray is pulled out towards the front.

4.6 Glass breakage

When centrifuging glass tubes, be aware that as speed/rcf increases, so the risk of glass breaking becomes greater. Please note the manufacturer's instructions pertaining to maximum load for centrifuge tubes. In the event of glass breakage, carefully remove all splinters and all ground glass from the rotor, the buckets, the adapters and the rotor chamber. You may need to replace the rubber plates and adapters to prevent further damage.

Fine splinters of glass may otherwise scratch the surface of the rotors and buckets, reducing their resistance to chemicals. The air eddies in the rotor chamber produce a very fine black cloud of abraded metal which, in addition to causing damage to the rotor chamber, rotor, buckets and adapters, also results in samples becoming contaminated.

Check the rotor bores regularly for residues and damage.

4.7 Return of the devices

When returning centrifuges, please ensure that the devices have been decontaminated and thereby do not present a health risk to our Service staff.

You will find additional information and a blank of the decontamination confirmation at www.eppendorf.com. Do also consult your laboratory safety officer about a suitable decontamination method.

Please fill out the decontamination confirmation and place it together with the device when it is to be sent back to Eppendorf.

5 Troubleshooting

Centrifuges 5417 C / R

Error	Display	Cause	Solution
No display.	None	No mains connection. Power failure.	Check power supply cable. Check main power fuse on the device and in the laboratory.
	CLEAn ro	200 runs.	Clean rotor.
Centrifuge does not start up.	Error 3	No rotor.	Insert rotor.
	Error 23	Error in the drive or rotor recognition.	Switch off the device and switch it on again.
Lid cannot be opened.	None	Power failure.	Bring rotor to a standstill, activate emergency lid release.
Lid not closed completely.	LID	Lid latch not engaged.	Press down lid again.
Centrifuge shakes during acceleration and switches off.	InbAL	Rotor not loaded symmetrically.	Check rotor loading.
	rotor	Rotor not fastened.	Fasten rotor correctly.
	SPEEd	Nominal speed too high.	Enter new nominal speed.
	Int	Power failure during the run.	Repeat run.
	Error 1	Rotor is not recognized.	Repeat run. If error recurs, test with another rotor.
	Error 2	Imbalance sensor defective.	Repeat run.
	Error 3	No rotor.	Insert rotor.
		Errors in rotational speed measuring system.	Leave device switched on for 8 min, then open the device. Repeat run.
	Error 5	Unauthorized opening of lid or lid switch defective.	Repeat run.
	Error 6	Converter overloaded. Brake defective.	Restart device after 5 min.
		Rotor loose.	Tighten rotor.
	Error 7	Overspeed.	Repeat run.
	Error 8	Rotor loose.	Tighten rotor.
		Drive error; motor defective.	⇒ SERVICE.
	Error 9–25	Electronics error.	⇒ SERVICE.
Flashing temperature display.		Temperature deviation from nominal value > 3 °C.	
Warning signal.	Error 18	Temperature deviation from nominal value > 5 °C.	The nominal value which has been set is too low or refrigeration is defective.

If the above solutions are unsuccessful, please contact SERVICE.

When an error display appears, press the Soft key and the Speed key above it at the same time and record the values displayed for servicing via remote diagnosis.

6 Technical data

Centrifuge 5417 C

Power supply:	230 V / 50–60 Hz 120 V / 50–60 Hz 100 V / 50–60 Hz
See identification plate	
Power requirement:	400 W
Max. rotational speed:	16,400 rpm
Max. centrifugal force:	25,000 rcf
Max. load:	30 x 2.0 ml Safe-Lock Microcentrifuge Tubes
Max. density of material to be centrifuged:	1.2 g/ml
Permitted ambient temperature during operation:	2 °C – 35 °C
Permitted maximum relative air humidity:	75 %
Max. kinetic energy:	6,100 Nm
Dimensions (H x W x D):	228 x 320 x 430 mm
Weight:	17 kg
Degree of pollution	2
Overvoltage category	II

Centrifuge 5417 R

Power supply:	230 V / 50 Hz or 60 Hz 120 V / 50 Hz or 60 Hz 100 V / 50 Hz or 60 Hz
See identification plate	
Power requirement:	
Centrifuge	400 W
Compressor	300 W
Max. rotational speed:	16,400 rpm
Max. centrifugal force:	25,000 rcf
Max. load:	30 x 2.0 ml Safe-Lock Microcentrifuge Tubes
Max. density of material to be centrifuged:	1.2 g/ml
Range of control for refrigeration:	– 9 °C to + 40 °C
Refrigeration time for "Fast Cool"	from 20 °C to 4 °C: approx. 20 min.
Permitted ambient temperature during operation:	10 °C–35 °C
Permitted maximum relative air humidity:	75 %
Max. kinetic energy:	6,100 Nm
Dimensions (H x W x D):	228 x 320 x 597 mm
Weight:	34 kg
Degree of pollution	2
Overvoltage category	II

Technical specifications subject to change!

7 Ordering information

Centrifuge 5417 C Microcentrifuge, Rotational speed regulation from 500 rpm to 16,400 rpm 230 V/50–60 Hz, without rotor Other voltage versions available on request!	5417 000.315
Centrifuge 5417 R Refrigerated microcentrifuge, Rotational speed regulation from 500 rpm to 16,400 rpm Temperature control from – 9 °C to 40 °C, 230 V/50 or 60 Hz, without rotor Other voltage versions available on request!	5407 000.317
Fixed-angle rotor F-45-30-11 incl. aluminium lid, 30 x 1.5/2 ml, max. rcf: 20,800	5490 015.002
Fixed-angle rotor FA-45-30-11 incl. aerosol-tight rotor lid, 30 x 1.5/2 ml, max. rcf: 20,800	5490 025.008
Fixed-angle rotor F-45-24-11 incl. aerosol-tight rotor lid, 24 x 1.5/2 ml, max. rcf: 25,000	5490 061.004
Swing-bucket rotor A-8-11 incl. aluminium lid, 8 x 1.5/2 ml	5492 008.003
PCR-tube strip rotor F-45-48-6-PCR 6 x 8-tube strips 6 x 5-tube strips 48 x 0.2 ml PCR test tubes	5490 060.008
Accessories	
Adapter for 0.5 ml micro test tubes and B-D Microtainer (set of 6) for F 45-30-11 and FA 45-30-11 (5 sets required) for swing-bucket rotor A 8-11 (2 sets required)	5425 716.001
Adapter for 0.4 ml centrifuge tubes (set of 6) for F 45-30-11 and FA 45-30-11 (5 sets required) for swing-bucket rotor A 8-11 (2 sets required)	5425 717.008
Adapter for 0.2 ml PCR test tubes (set of 6)	5425 715.005
Buckets for swing-bucket rotor 8 x 1.5/2.0 ml (set of 12)	5498 000.012
Rotor lid for F 45-30-11 (aluminium)	5490 004.302
Rotor lid for aerosol-tight rotor FA 45-30-11	5490 025.806
Rotor lid for aerosol-tight rotor FA 45-24-11	5425 734.000
Rotor lid for A 8-11	5492 006.302
O-ring for rotor F 45-30-11	5498 900.137


Magnetic ring for fixed-angle rotor F-45-30-11 / FA-45-30-11	5498 900.102
Magnetic ring for swing-bucket rotor	5498 900.110
Magnetic ring for fixed-angle rotor F-45-24-11	5490 010.205
Microfuses (set of 2)	
for 5417 R 230 V / 2 x 6.3 A, T	5417 341.007
for 5417 R 120 V / 10.0 A, T UL	5407 357.000
for 5417 R 100 V / 12.0 A, mT UL	5407 356.006
for 5417 C 230 V / 2 x 6.3 A, T	5417 341.007
for 5417 C 120 V / 8.0 A, T UL	5417 356.004
for 5417 C 100 V / 10.0 A, T UL	5417 357.000
Hexagonal key	5416 301.001
Mains cable (230 V)	0013 563.934
Mains cable (US 115 V)	0013 563.942

Important note:

Please use the original accessories recommended by Eppendorf. Using spare parts or disposables which we have not recommended can reduce the precision, accuracy and life of the centrifuges. We do not honor any warranty or accept any responsibility for damage resulting from such action.

Rotor code

All Eppendorf rotors are designated according to a simple, logical system which describes the technical specifications as a uniform series of numbers and letters e.g.:

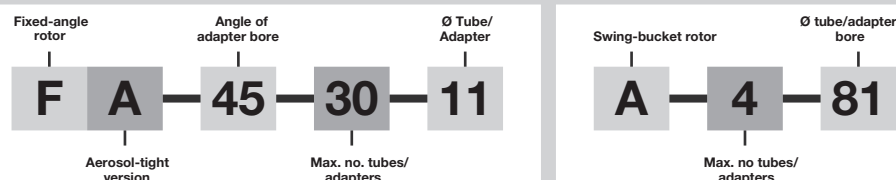

8 Appendix

Calculation of rcf

The maximum relative centrifugal force (rcf) stated as a multiple of the gravitational force "g" can be calculated for each tube from the rotational speed n (rpm) and the maximum radius of centrifugation r (cm).

$$rcf = 11.18 \times r \times (n/1\,000)^2$$

In rotor F 45-30-11, the following maximum radii of centrifugation and rcf are valid for the various micro test tubes:

<i>Tube type</i>	<i>at n (rpm)</i>	<i>r (cm)</i>	<i>rcf</i>
2.0 ml Safe-Lock Microcentrifuge Tube	14,000	9.5	20,800
1.5 ml Safe-Lock Microcentrifuge Tube, 3810	14,000	9.2	20,200
0.5 ml Safe-Lock Microcentrifuge Tube	14,000	8.3	18,200
0.4 ml Centrifuge Tube	14,000	9.2	20,200
1.7 ml Safe-Twist Screw Cap Tube	14,000	9.2	20,200

This conversion table is valid for 2.0 ml Safe-Lock Microcentrifuge Tubes in a fixed-angle rotor:

<i>rpm</i>	<i>in</i>	<i>rcf</i>
1 000		110
2 000		420
3 000		960
4 000		1 700
5 000		2 700
6 000		3 800
7 000		5 200
8 000		6 800
9 000		8 600
10 000		10 600
11 000		12 900
12 000		15 300
13 000		17 900
14 000		20 800

Eppendorf Offices

AUSTRALIA / NEW ZEALAND

Eppendorf South Pacific Pty. Ltd.
Tel. +61 2 98 89 50 00
Fax +61 2 98 89 51 11
E-Mail: Info@eppendorf.com.au
Internet: www.eppendorf.com.au

AUSTRIA

Eppendorf Austria
Tel. +43 1 2901756-0
Fax +43 1 2901756-20
E-Mail: office@eppendorf.at
Internet: www.eppendorf.at

BRAZIL

Eppendorf do Brasil Ltda.
Tel. +55 11 3095 9344
Fax +55 11 3095 9340
E-Mail: eppendorf@eppendorf.com.br
Internet: www.eppendorf.com.br

CANADA

Eppendorf Canada Ltd.
Tel. +1 905 826 5525
Fax +1 905 826 5424
E-Mail: canada@eppendorf.com
Internet: www.eppendorfna.com

CHINA

Eppendorf China Ltd.
Tel. +86 21 68760880
Fax +86 21 50815371
E-Mail: market.info@eppendorf.cn
Internet: www.eppendorf.cn

CZECH REP. & SLOVAKIA

EPPENDORF Czech & Slovakia s.r.o.
Tel. +420 323 605 454
Fax +420 323 605 454
E-Mail: eppendorf@eppendorf.cz
Internet: eppendorf.cz
Internet: eppendorf.sk

FRANCE

EPPENDORF FRANCE S.A.R.L.
Tel. +33 1 30 15 67 40
Fax +33 1 30 15 67 45
E-Mail: eppendorf@eppendorf.fr
Internet: www.eppendorf.fr

GERMANY

Eppendorf Vertrieb
Deutschland GmbH
Tel. +49 2232 418-0
Fax +49 2232 418-155
E-Mail: vertrieb@eppendorf.de
Internet: www.eppendorf.de

INDIA

Eppendorf India Limited
Tel. +91 44 42 11 13 14
Fax +91 44 42 18 74 05
E-Mail: info@eppendorf.co.in
Internet: www.eppendorf.co.in

ITALY

Eppendorf s.r.l.
Tel. +390 2 55 404 1
Fax +390 2 58 013 438
E-Mail: eppendorf@eppendorf.it
Internet: www.eppendorf.it

JAPAN

Eppendorf Co. Ltd.
Tel. +81 3 5825 2363
Fax +81 3 5825 2365
E-Mail: info@eppendorf.jp
Internet: www.eppendorf.jp

NORDIC

Eppendorf Nordic Aps
Tel. +45 70 22 29 70
Fax +45 45 76 73 70
E-Mail: nordic@eppendorf.dk
Internet: www.eppendorf.dk

SOUTH & SOUTHEAST ASIA

Eppendorf Asia Pacific Sdn. Bhd.
Tel. +60 3 8023 2769
Fax +60 3 8023 3720
E-Mail: eppendorf@eppendorf.com.my
Internet: www.eppendorf.com.my

SPAIN

Eppendorf Ibérica S.L.U.
Tel. +34 91 651 76 94
Fax +34 91 651 81 44
E-Mail: iberica@eppendorf.es
Internet: www.eppendorf.es

SWITZERLAND

Vaudaux-Eppendorf AG
Tel. +41 61 482 1414
Fax +41 61 482 1419
E-Mail: vaudaux@vaudaux.ch
Internet: www.eppendorf.ch

UNITED KINGDOM

Eppendorf UK Limited
Tel. +44 1223 200 440
Fax +44 1223 200 441
E-Mail: sales@eppendorf.co.uk
Internet: www.eppendorf.co.uk

USA

Eppendorf North America, Inc.
Tel. +1 516 334 7500
Fax +1 516 334 7506
E-Mail: info@eppendorf.com
Internet: www.eppendorfna.com

OTHER COUNTRIES

Internet:
www.eppendorf.com/worldwide



Fig. 5



Fig. 6



Fig. 7

EG-Konformitätserklärung EC Conformity Declaration

Das bezeichnete Produkt entspricht den einschlägigen grundlegenden Anforderungen der aufgeführten EG-Richtlinien und Normen. Bei einer nicht mit uns abgestimmten Änderung des Produktes oder einer nicht bestimmungsgemäßen Anwendung verliert diese Erklärung ihre Gültigkeit.

The product named below fulfills the relevant fundamental requirements of the EC directives and standards listed. In the case of unauthorized modifications to the product or an unintended use this declaration becomes invalid.

Produktbezeichnung, Product name:

Centrifuge 5417 C / R

einschließlich Zubehör / including accessories

Produkttyp, Product type:

Laborzentrifuge / Laboratory Centrifuge

Einschlägige EG-Richtlinien/Normen, Relevant EC directives/standards:

2006/95/EG, EN 61010-1, EN 61010-2-20

2004/108/EG, EN 55011/B, EN 61000-6-1, EN 61000-3-2, EN 61000-3-3, EN 61326

98/37/EG, EN 292-2, EN 292-2/A1,

98/79/EG, EN 14971, EN 61010-2-101



Vorstand / Board of Management:

21.05.2007

Hamburg, Date:



Projektmanagement, Project Management:



eppendorf

Eppendorf AG · Barkhausenweg 1 · 22339 Hamburg · Germany

0015 033.509-02

5417 900.308-09

Your local distributor:
www.eppendorf.com/worldwide

Eppendorf AG
22331 Hamburg · Germany
Tel. +49 40 538 01-0
Fax +49 40 538 01-556
E-mail: eppendorf@eppendorf.com
Eppendorf North America, Inc.
One Cantiague Road, P.O. Box 1019
Westbury, N.Y. 11590-0207 · USA
Tel. +1 516 334 7500
Toll free phone +1 800 645 3050
Fax +1 516 334 7506
E-mail: info@eppendorf.com

Application Support
Europe, International:
Tel. +49 1803 666 789
E-mail: support@eppendorf.com
North America:
Tel. +1 800 645 3050 ext. 2258
E-mail: support_na@eppendorf.com
Asia Pacific:
Tel. +60 3 8023 6869
E-mail:
support_asiapacific@eppendorf.com

eppendorf